



Guide to interpret ATP-metry values - Swimming pool surfaces -

Pool opening (results in LOG/cm²):

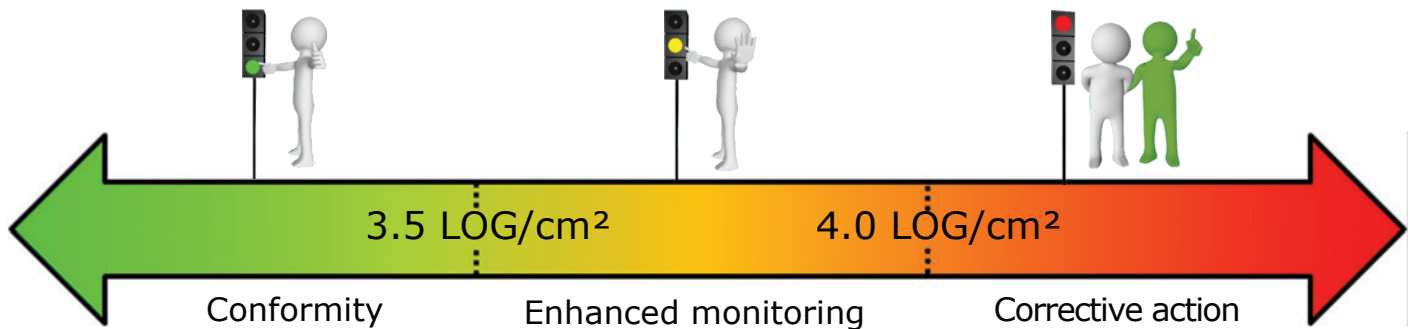

Operating swimming pools (results in LOG/cm²):

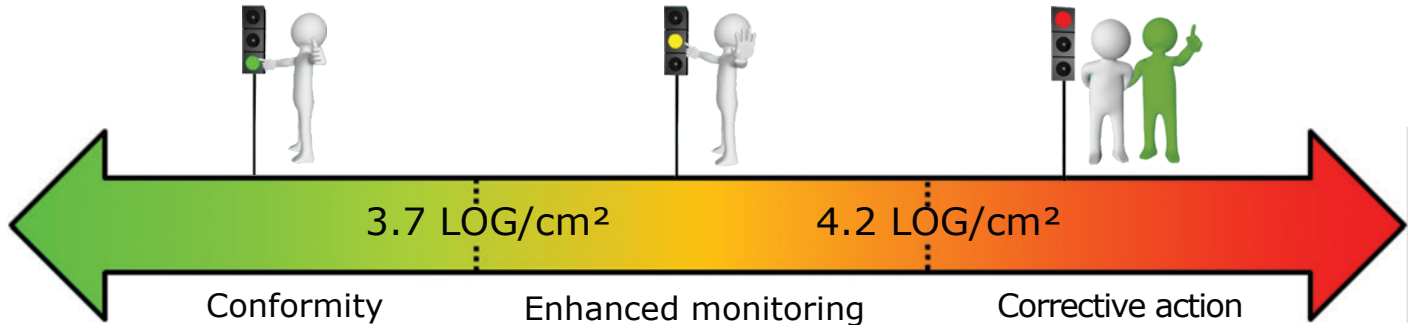

These thresholds were determined in collaboration with the French ARS (Regional Health Agencies). We consider that when a measurement is:

- **Below the warning threshold (conformity)**, the surface is clean and under control,
- **Between the warning threshold and alarm threshold (enhanced monitoring)**, the surface does not present an immediate biohazard. A corrective action is recommended,
- **Above the alarm threshold (corrective action)**, the surface is not under control. A quick corrective action is recommended (cleaning, disinfection...).